

(12)特許協力条約に基づいて公開された国際出願

(19) 世界知的所有権機関
国際事務局(43) 国際公開日
2005年8月4日 (04.08.2005)

PCT

(10) 国際公開番号
WO 2005/071420 A1(51) 国際特許分類: G01N 33/68, C12Q
1/34, G01N 21/77, 21/78, 21/82, 33/70

(21) 国際出願番号: PCT/JP2005/000758

(22) 国際出願日: 2005年1月21日 (21.01.2005)

(25) 国際出願の言語: 日本語

(26) 国際公開の言語: 日本語


(30) 優先権データ:
特願2004-016146 2004年1月23日 (23.01.2004) JP(71) 出願人(米国を除く全ての指定国について): アーク
レイ株式会社 (ARKRAY, INC.) [JP/JP]; 〒6018045 京
都府京都市南区東九条西明田町5-7 Kyoto (JP).

(72) 発明者; および

(75) 発明者/出願人(米国についてのみ): 小坂 秀子
(KOSAKA, Hideko) [JP/JP]; 〒6018045 京都府京都市
南区東九条西明田町5-7 アークレイ株式会社内
Kyoto (JP). 坂本 久 (SAKAMOTO, Hisashi) [JP/JP]; 〒
6018045 京都府京都市南区東九条西明田町5-7 アー
クレイ株式会社内 Kyoto (JP).(74) 代理人: 吉田 稔, 外(YOSHIDA, Minoru et al.);
〒5430014 大阪府大阪市天王寺区玉造元町2番
3-2-1301 Osaka (JP).(81) 指定国(表示のない限り、全ての種類の国内保護が
可能): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR,
BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM,
DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU,
ID, IL, IN, IS, JP, KB, KG, KP, KR, KZ, LC, LK, LR, LS,
LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA,
NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE,
SI, SK, SL, SM, SN, SR, ST, SV, SY, TD, TH, TJ, TM, TN,
TR, TT, TZ, UA, UG, US, UZ, VC, VE, VN, YU, ZA, ZM, ZW.
(続表有)

(54) Title: METHOD OF PROTEIN MEASUREMENT

(54) 発明の名称: 蛋白質測定方法

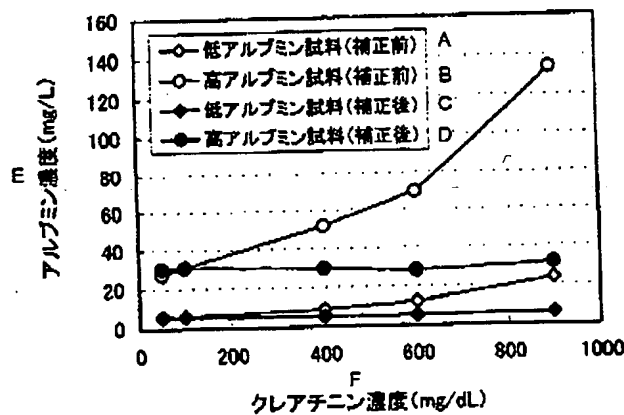

A ... LOW ALBUMIN SAMPLE (BEFORE CORRECTION)
B ... HIGH ALBUMIN SAMPLE (BEFORE CORRECTION)
C ... LOW ALBUMIN SAMPLE (AFTER CORRECTION)
D ... HIGH ALBUMIN SAMPLE (AFTER CORRECTION)
E ... ALBUMIN CONCN. (mg/L)
F ... CREATININE CONCN. (mg/dL)

(57) Abstract: A technique for performing protein measurement on the basis of the level of coloring upon coexistence of a liquid sample with an indicator for protein measurement. In this technique, information reflecting the concentration of creatinine in a liquid sample is procured, and in accordance with this information, the amount of creatinine influence on the measurement of protein concentration is removed.

(続表有)

WO 2005/071420 A1

INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2005/000758

A. CLASSIFICATION OF SUBJECT MATTER

Int.Cl.⁷ G01N33/68, C12Q1/34, G01N21/77, 21/78, 21/82, 33/70

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

Int.Cl.⁷ G01NN33/48-33/98

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Jitsuyo Shinan Koho	1922-1996	Toroku Jitsuyo Shinan Koho	1994-2005
Kokai Jitsuyo Shinan Koho	1971-2005	Jitsuyo Shinan Toroku Koho	1996-2005

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
CA

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X/Y	JP 11-190735 A (Bayer Corp.), 13 July, 1999 (13.07.99), (Claims; Par. Nos. [0001], [0002], [0007]) & EP 0909953 A2	1-6, 8, 15-17 /7, 9-14
Y	JP 2002-116203 A (Nitto Denko Corp.), 19 April, 2002 (19.04.02), (Claims; Par. No. [0011]) (Family: none)	7, 11, 14
Y	WAHEED, A.A. et al., Mechanism of dye binding in the protein assay using eosin dyes. Analytical Biochemistry, 2000, vol.287, pages 73 to 79. (Abstract Sansho)	7, 11-13

☒ Further documents are listed in the continuation of Box C.☐ See patent family annex.

* Special categories of cited documents:

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier application or patent but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

G document member of the same patent family

Date of the actual completion of the international search
14 February, 2005 (14.02.05)Date of mailing of the international search report
01 March, 2005 (01.03.05)Name and mailing address of the ISA/
Japanese Patent Office

Authorized officer

Facsimile No.

Telephone No.

INTERNATIONAL SEARCH REPORT

International application No.

PCT/JP2005/000758

C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	JP 07-198719 A (Miles Inc.), 01 August, 1995 (01.08.95), (Claims) & US 5385847 A	9,10
Y	HONG H-Y. et al., An eosin Y method for protein determination in solution. Analytical Letters, 1999. Vol.32(12), pages 2427 to 2442. (Abstract Sansho)	7,11-13
A	JP 09-079982 A (Kyoto Daiichi Kagaku Co., Ltd.), 28 March, 1997 (28.03.97), & EP 0751388 A3	1-17
A	JP 02-122264 A (Miles Inc.), 09 May, 1990 (09.05.90), & US 5049358 A & EP 0361244 A2	7,11-13
A	JP 05-209836 A (Terumo Corp.), 20 August, 1993 (20.08.93), (Family: none)	1-17
A	FORKER, E.L. et al., Hepatic transport and binding of rose bengal in the presence of albumin and gamma globulin. American J. Physiol., 1985. Vol.248(6, Pt.1), pages G702 to G708.	7,11-13

SPECIFICATION

METHOD OF PROTEIN MEASUREMENT

5 FIELD OF THE INVENTION

The present invention relates to a technique for measuring a protein contained in a liquid sample.

BACKGROUND ART

10 Blood contains many kinds of proteins essential for supporting life. Of these proteins, albumin occupies the largest part in quantity and has many important functions.

Albumin in the blood makes fat soluble, while making a bond with substances harmful to living organism, thereby
15 carrying these substances to the liver. Further, albumin plays an important role in maintaining the blood osmotic pressure. Albumin is also present in urine by a very small amount. The amount of albumin in urine reflects, for example, the level of filtering function of the glomeruli in the kidneys.

20 An increase in the amount of urinary albumin indicates that the filtering function of the glomeruli in the kidneys may have deteriorated. If the increase of urinary albumin is not taken care of, one may suffer albuminuria, which is often symptomatic of kidney disease such as chronic nephritis. If
25 such a disease is found, dialysis must be performed, and much worse, the patient may have kidney implanting surgery. In light of these, it is important to monitor the amount of albumin in urine so that a malfunction of the kidney can be found at an early stage.

As a technique which is usable for measurement of protein such as albumin, there is a simple measurement method called immunochromatography (see Patent Documents 1 and 2). The method is carried out by using an analytical element or a capillary strip containing a labeled antibody provided in a first region and a capture antibody (anti-albumin antibody) provided in a second region. More specifically, a liquid sample (urine for example) is supplied to the first region, whereupon capillary action of the strip causes the labeled antibody and the liquid sample to move to the second region. If the liquid sample contains the detection target antigen (albumin), the antigen combines with the labeled antibody as being moved to the second region. At the second region, the antigen-antibody combination is captured by the capture antibody. Then, based on the coloring of the antigen-antibody combination in the second region, it is possible to make a visual, qualitative determination on whether or not the urine contains a greater amount of protein than a predetermined level.

20 The immunochromatography is a qualitative method that enables visual determination of whether the result is negative or positive, so it is useful as a preliminary check for a functional impairment in the kidney. However, the immunochromatography is disadvantageous in that it cannot specify the level of the renal impairment quantitatively. In addition, the measurement takes a long time, often 10 - 15 minutes, until the liquid sample has completed its movement along the strip.

On the other hand, simple quantitative methods have been

proposed for measuring the protein concentration. Well known examples are protein error method and dye binding method (see Patent Documents 3 and 4). The protein error method makes use of a phenomenon that a pH indicator called protein error
5 indicator gives a color at a higher pH than the true pH, in proportion to the amount of protein contained in the sample. The dye binding method, on the other hand, makes use of a phenomenon that a maximum absorption wavelength of a dye shifts when the dye is combined with protein.

10 The protein error method and the dye binding method are highly convenient because they are simple methods to use. On the contrary, accurate measurement of protein is difficult in the protein error method and the dye binding method because the reagents used commonly in these measurement methods do
15 not have high specificity to urinary albumin and therefore affected by a number of substances which are present in the urine. To date, various improvement efforts have been made for the protein error method and the dye binding method in order to increase measurement accuracy for example. Yet,
20 there is still room for improvement in the protein error method and the dye binding method in the field of measurement accuracy for example.

There are methods which are less susceptible to influences from coexisting substances in urine. Examples include use
25 of metal colloid (see Patent Document 5 for example), immunoturbidimetric method, and immunolateral agglutination method. In the colloidal metal method, a membrane is used to absorb protein. The membrane is then washed to remove coexisting substances. Then metal colloid is combined with

the protein to determine quantity of the protein from the color of the metal colloid. The method is certainly less susceptible to influences from the coexisting substances, but is disadvantageous in that it requires complicated measurement operations such as the step of adsorbing protein in a membrane, the step of washing, and the step of allowing the metal colloid to combine with the protein. On the other hand, the immunoturbidimetric method and the immunolateral agglutination method are disadvantageous in terms of measurement cost since they require expensive reagents.

Patent Document 1: JP-B-H07-13640

Patent Document 2: JP-A-H10-73592

Patent Document 3: JP-B-S57-51627

Patent Document 4: JP-A-S61-155757

Patent Document 5: JP-A-S63-127160

DISCLOSURE OF THE INVENTION

An object of the present invention is to provide an easy, cost-advantageous and accurate method for quantifying a protein (e.g. albumin) in a liquid sample.

In order to achieve the above-described object, diligent examinations were made by the inventors. As a result, the inventors found that in albumin quantification using a specific protein measurement indicator, creatinine and albumin show similar behavioral patterns to this protein measurement indicator. In other words, the present invention is based on this finding that creatinine reacts with a specific protein measurement indicator, thereby functioning as an error factor, influencing the quantification of albumin.

Specifically, the present invention provides a method for measuring a concentration of a protein (e.g. albumin) in a liquid sample (e.g. urine, blood and cerebrospinal fluid). In this method, information which reflects an influence of the creatinine concentration in the liquid sample is obtained, and then, based on this information, the influence of creatinine on the protein concentration measurement is eliminated.

The method of measuring a protein according to the present invention includes: a first step of obtaining a first response value which is correlated with a protein concentration in the liquid sample, based e.g. on coloring given by a system containing the liquid sample and a protein measurement indicator; a second step of obtaining a second response value which is correlated with a creatinine concentration in the liquid sample in a system containing the liquid sample but not containing the protein measurement indicator; and a third step of calculating a concentration of the protein in the liquid sample, taking the second response value into consideration and based on the first response value.

Here is a specific method of eliminating the influence caused by the amount of creatinine. For example, in the second step, an influence caused by the amount of creatinine to the first response value is calculated based on the second response value, and then in the third step, a protein concentration is calculated as a preliminary value based on the first response value, and then a final protein concentration is calculated by subtracting the influence quantity of the amount of creatinine from the preliminary value. Another method of

eliminating the influence caused by the amount of creatinine is as follows: In the third step, a corrected response value is obtained by correcting the first response value based on the first and the second response values, and then a protein
5 concentration in the liquid sample is calculated based on the corrected response value.

It is noted here that the method of measuring a protein according to the present invention provides an example, in which a creatinine concentration is measured, and then a final
10 protein concentration is calculated based on this creatinine concentration. This process is different from conventional creatinine correction.

Specifically, the conventional creatinine correction equalizes a difference in measuring condition caused by
15 dilution or concentration of urine for example, when the liquid sample is urine. More specifically, the albumin concentration is divided by the creatinine concentration to obtain protein concentrations under a hypothetical, universal measuring condition. On the contrary, according to the method
20 of measuring a protein offered by the present invention, an increase in the first response value caused by creatinine's reaction with the protein measuring reagent is grasped by measuring the creatinine concentration, separately from the dilution/concentration problem. Then the amount of increase
25 is virtually offset from the response value, and the protein measurement is based on this response value. In other words, a creatinine concentration obtained for the conventional purpose of creatinine correction can be used as a creatinine concentration for the method of measuring a protein according

to the present invention.

According to the present invention, a creatinine concentration (or a response which is correlated with the creatinine concentration) in a liquid sample is grasped, and
5 then the influence on the protein concentration by the creatinine concentration is eliminated. Therefore, according to the present invention, it is possible to obtain accurate measurements without creatinine influence, by an easy and cost-advantageous method using a protein measurement
10 indicator.

BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a graph showing a relationship between reflection coefficients measured by protein error method and protein
15 concentrations measured by a pyrogallol red method.

Fig. 2 is a graph showing calculated values of protein concentration before and after eliminating creatinine influences.

Fig. 3 is a graph showing a relationship between reflection
20 coefficients measured by a dye binding method and albumin concentrations measured by an immunoturbidimetric method.

Fig. 4 is a graph showing how the amount of creatinine influences on reflection coefficient measurements, demonstrated by using a low-albumin sample and a high-albumin
25 sample.

Fig. 5 is a graph showing calculated values of albumin concentration before and after eliminating creatinine influence, demonstrated by using a low-albumin sample and a high-albumin sample.

Fig. 6 is a graph showing a relationship between reflection coefficients when creatinine concentration is 100 mg/dL and absolute values of gradient in the graph in Fig. 4.

5 BEST MODE FOR CARRYING OUT THE INVENTION

The present invention relates to a technique for eliminating the influence of creatinine on a protein measurement which is based on coloring of a liquid sample coexisting with a protein measurement indicator.

10 Specifically, according to the protein measuring method of the present invention, information reflecting creatinine concentration in the liquid sample is obtained, and then, based on this information, the influence of creatinine on the measurement of the protein concentration is eliminated. The

15 present invention is applicable to liquid samples of urine, blood, and cerebrospinal fluid for example. The present invention is also applicable to any protein-containing liquid, such as a protein beverage and industrial wastewater. A typical example of protein as the target of measurement

20 according to the present invention is albumin. Besides albumin, other proteins such as globulin and Bence-Jones protein can be measured by the present invention.

The method of measuring a protein according to the present invention includes: a first step of obtaining a first response


25 value which reflects a protein concentration in a liquid sample, based e.g. on coloring given by a system in which the liquid sample and a protein measurement indicator coexist; a second step of obtaining a second response value which reflects a creatinine concentration in the liquid sample in a system

containing the liquid sample but not any protein measurement indicator; and a third step of calculating the concentration of the protein in the liquid sample. This calculation is conducted in consideration of the second response value and
5 based on the first response value.

In the first step, the first response value is obtained through a first protein measurement procedure (e.g. dye binding method or protein error method).

The dye binding method in the present invention refers
10 to a method of measuring a protein which utilizes a phenomenon that protein bound with a dye (indicator) shifts the dye's maximum absorption wavelength. Examples of the dye include halogenated xanthene dyes and Coomassie Brilliant Blue. Among these indicators, it is preferable to use a halogenated
15 xanthene dye. Usable halogenated xanthene dyes have the chemical structure expressed by Chemical Formula 1.

Chemical Formula 1

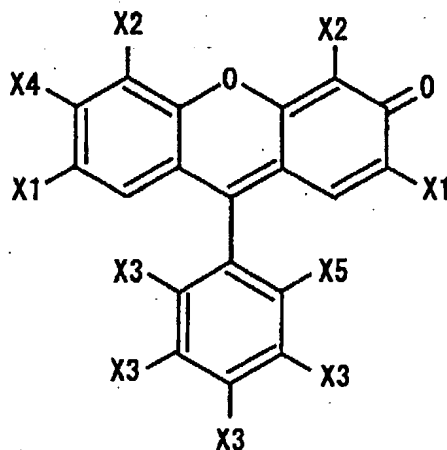




In Chemical Formula 1, X1 represents a halogen, a nitro group or a nitroso group, X2 represents a halogen, X3 represents a halogen or hydrogen, X4 represents a hydroxyl group or its salt, X5 represents a carboxyl group or its salt.



5 Preferred halogenated xanthene dyes according to the present invention are those expressed by Chemical Formula 1, with X1 provided by iodine, bromine, chlorine or a nitro group, X2 provided by iodine or bromine, X3 provided by chlorine, bromine or hydrogen. The most preferred are those with X1
10 and X2 provided by iodine or bromine, and X3 provided by chlorine. Examples of salt for X4 and X5 are sodium salts typically.

Preferred halogenated xanthene dyes according to the present invention are those expressed by Chemical Formulas 2 through 6. In particular, it is preferable to use protein
15 measurement indicators expressed by Chemical Formulas 2 and 3.

Chemical Formula 2

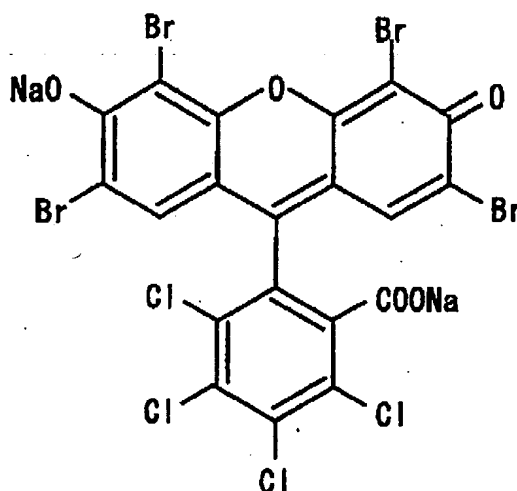

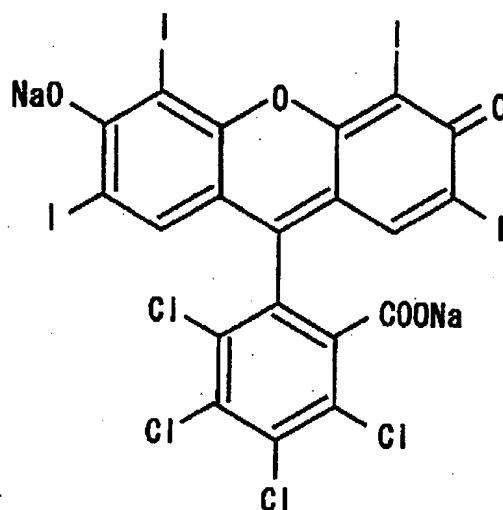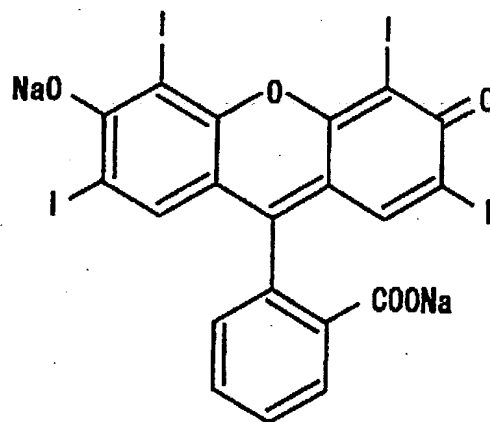Chemical Formula 35 Chemical Formula 4

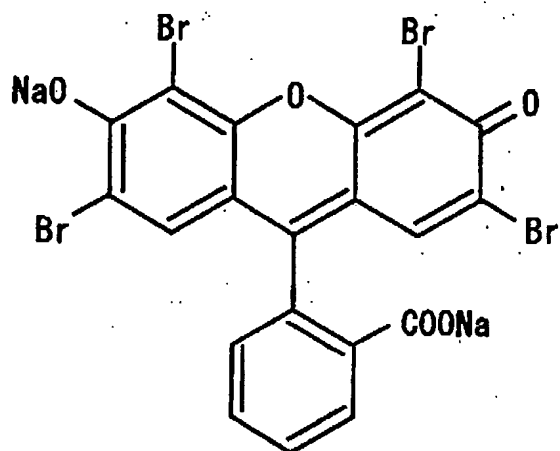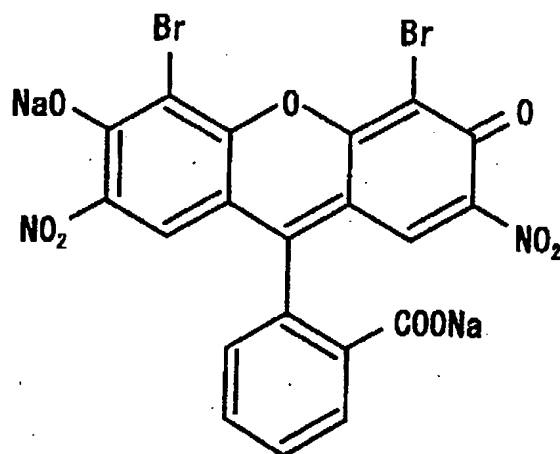Chemical Formula 55 Chemical Formula 6

The halogenated xanthene dyes represented by Chemical Formulas 2 through 6 can be obtained easily from the manufacturers listed in Table 1.

5 Table 1

	Brand Name	Manufacturer
Chemical Formula 2	Phloxine B	Tokyo Chemical Industry Co., Ltd. (Japan)
Chemical Formula 3	Rose Bengal	Tokyo Chemical Industry Co., Ltd. (Japan)
Chemical Formula 4	Erythrosine B	Tokyo Chemical Industry Co., Ltd. (Japan)
Chemical Formula 5	Eosin Y	Wako Pure Chemical Industries, Ltd. (Japan)
Chemical Formula 6	Eosin B	Tokyo Chemical Industry Co., Ltd. (Japan)

The protein error method in the present invention refers to a method of measuring a protein which utilizes a phenomenon that a protein error indicator, which is a type of pH indicator, gives a color at a higher pH than the true pH in proportion to the amount of protein contained in the sample. Examples of the protein error indicator are triphenylmethane dyes. Specific examples of the triphenylmethane dyes include Tetrabromophenol Blue (TBPB), Bromochlorophenol Blue (BCPB), and Bromophenol Blue (BPB), with Tetrabromophenol Blue (TBPB) being most typical.

In the second step of the present invention, the second response value is measured in accordance with e.g. enzyme method, Jaffe method, copper chelate oxidation method, palladium complex competition method, or Benedict method.

The enzyme method is a method of measuring creatinine from the amount of a product created by reaction between creatinine

and an enzyme. Examples of the enzyme used in this method include creatinine deaminase and creatinine amidohydrolase (creatininase). When the former enzyme is used, ammonia is generated from creatinine by the activity of creatinine deaminase, and the amount of creatinine is measured from the amount of ammonia. On the other hand, when the latter enzyme is used, creatine is generated from creatinine by the activity of creatinine amidohydrolase (creatininase), and the amount of creatinine is measured from the amount of creatine. The amount of creatinine is measured by causing the creatine to act with creatine amidohydrolase, sarcosine oxidase and peroxidase, thereby producing hydrogen peroxide, and then the hydrogen peroxide is led to a coloring system for measurement of the creatine.

Jaffe method is a method of measuring creatinine by measuring the brown coloration caused by a reaction between creatinine and picric acid under alkaline conditions.

The copper chelate oxidation method is a method of measuring creatinine by utilizing a reaction in which copper and creatinine form a complex under neutral conditions, showing peroxidase activity.

The palladium complex competition method is a method of measuring creatinine based on a change in a dye's maximum absorption wavelength when a complex between palladium and the dye is present with creatinine. The method is detailed in the JP-A 2004-138407 Gazette. An example of the dye which is to be used for this method is Chromazurol S (2,6-Dichloro-4'-hydroxy-3',3''-dimethylfuchsone-5',5''-dicarboxylic acid, disodium salt).

The Benedict method is a method of quantifying creatinine by utilizing a reaction (Benedict reaction) between Benedict's reagent and creatinine under alkaline conditions.

In the third step, the protein concentration is calculated
5 based on a predetermined calibration curve. The calibration curve can be made by a method which includes: a step of obtaining a plurality of responses for each of a plurality of liquid samples, based on a first protein measurement procedure; a step of measuring a protein concentration in each of the liquid
10 samples based on a second protein measurement procedure which is less susceptible to creatinine influence than the first protein measurement procedure; and a step of relating the responses to the protein concentrations measured by the second protein measurement procedure.

15 Examples of the second protein measurement procedure include immunoturbidimetric method, immunol latex agglutination method, and ternary complex method.

The immunoturbidimetric method is a method of measuring an antigen (protein) based on turbidity caused by a lattice
20 crystal formed in a reaction between the antigen (protein) and its antibody. The antibody is selected in accordance with the kind of target protein for the measurement. For example, when measuring albumin, a monoclonal antibody or a polyclonal antibody is used.

25 The immunol latex agglutination method is a method of measuring a protein based on turbidity caused by flocculant production formed in a reaction between the protein and an immune reactant which is specially reactive thereto and is born by latex microparticles.

The ternary complex method is a method of measuring a protein based on the color of a dye-metal complex, in a reaction between the protein and the complex. Examples of the metal which forms a complex with dye include indium, molybdenum, 5 cobalt, copper, and nickel.

Examples of the dye which forms a complex with indium include polyhydroxybenzene sulfonephthalein dyes and polyhydroxybenzene phthalein dyes. Typical examples are pyrocatechol violet, pyrogallol red, Bromopyrogallol red, 10 xylenol orange, pyrogallol phthalein and o-hydroxyhydroquinone phthalein.

Examples of the dyes which form a complex with molybdenum complex includes: pyrogallol red, Bromopyrogallol red, o-hydroxyhydroquinone phthalein and gallein.

15 In the method of measuring a protein according to the present invention, the second step includes, for example, calculation based on the second response value, of the influence quantity of the amount of creatinine to the first response value whereas the third step includes calculation 20 based on the first response value, of a preliminary value of the protein concentration, and calculation of a final protein concentration by subtracting the influence quantity of the amount of creatinine from the preliminary value.

In the second step, the creatinine influence quantity is 25 calculated, based on a predetermined calibration curve. The calibration curve can be made by, for example, first measuring response values from a plurality of liquid samples having the same protein concentration but different creatinine concentration from each other, using the above-described first

protein measurement procedure such as the dye binding method or the protein error method, and then relating these response values to the creatinine concentrations.

In the method of measuring a protein according to the present invention, the third step may include: obtainment of
5 a corrected response value by correcting the first response value based on the first and the second response values; and calculation of the protein concentration in the liquid sample, based on the corrected response value.

10 The corrected response value is calculated by arithmetic expression derived, for example, from a plurality of sample groups: Each sample group consists of a plurality of liquid samples having the same protein concentration but different creatinine concentration from each other, and each sample group
15 has a different protein concentration from each other. The arithmetic expression is derived from a method which includes for example: a step of measuring a response value for each of the liquid samples in each sample group; a step of obtaining a relationship between the response values from the liquid
20 samples and the creatinine concentrations in each sample group, as a plurality of relational expressions for all of the sample groups in the form of linear expression; and a step of obtaining a relationship between a gradient in each of the relational expressions and the response value from the liquid sample
25 having a specific creatinine concentration in each sample group, in the form of relational expression.

When practicing the present measurement method, the liquid sample is supplied to a liquid reagent containing the protein measurement indicator, or to a solid reagent containing the

protein measurement indicator. Preferably, however, the method in which the liquid sample is supplied to a solid reagent is used since it will help establishing an easier measurement procedure. A typical example of the solid reagent is one
5 carried by test paper.

The test paper can be made by impregnating an absorbing carrier with an impregnating solution containing the reagent, a buffer and so on, and then drying the impregnated carrier. The test paper piece may be used as is or otherwise; e.g. as
10 attached to a non-absorbent carrier formed of a synthetic resin for example.

There is no specific limitation to the concentration of the indicator in the impregnating solution. The concentration may depend on the kind of indicator used. A
15 typical concentration range is 0.1 through 10 mM, and more preferably 0.5 through 2 mM.

The impregnating solution has a pH value slightly lower than the pKa value of the indicator. For example, if the indicator is provided by a halogenated xanthene dye, the
20 solution should be in the range of pH=1.5 through 4.5, and more preferably of pH=2.0 through 3.5.

The buffer may be anything as long as it has a good buffering ability under the impregnating solution pH (e.g. pH=1.5 through 4.5), and does not inhibit the reaction between the protein
25 measuring reagent and the protein. Examples of the buffer include glycine buffer solution, citric acid buffer solution, succinic acid buffer solution, malic acid buffer solution and tartaric acid buffer solution. There is no specific limitation to the concentration of the buffer in the

impregnating solution. A typical concentration range is 0.1 through 1.5 M, and more preferably 0.3 through 1 M.

The absorbent carrier can be provided by a porous material which does not contain protein. The porous material may be
5 in the form of paper, foam (polyfoam), woven cloth, non-woven cloth or knitted work. Materials for forming the absorbent carrier include cotton, linen, cellulose, cellulose nitrate, acetylcellulose, rock wool, glass fiber, silica fiber, carbon
10 fiber, boron fiber, polyamide, aramid, polyvinyl alcohol, polyvinyl acetate, rayon, polyester, nylon, polyacrylic acid, polyacrylic acid ester, and polyolefin for example.

Example 1

In the present example, liquid samples of different protein
15 concentrations were dripped to test paper impregnated with a protein error indicator, to obtain reflection coefficients. Comparative study was made between the reflection coefficient and the protein concentration of each liquid sample measured by a pyrogallol red method, which is one of the ternary complex
20 methods.

The test paper was made by impregnating a filter paper (3MMChr, manufactured by Whatman plc), with an impregnating solution prepared by mixing 0.5 mM tetrabromophenol blue (TBPB), 0.5 M malic acid buffer solution (pH=3.4) and 30 wt%
25 ethanol, and then drying the paper. The reflection coefficients were measured by colorimeter, based on a reflected light when the test paper was irradiated with a light whose peak wavelength was 630 nm.

The liquid samples were made by adding an appropriate amount

of human serum albumin to low-creatinine-concentration, healthy-human urine which had a creatinine concentration not higher than 20 mg/dL. The amount of the liquid sample dripped to the test paper was 7 μ L.

- 5 Results of the measurements on the reflection coefficients and the protein concentrations are given in Fig. 1, where the reflection coefficient is represented by the horizontal axis and the protein concentration is represented by the vertical axis. As understood from Fig. 1, there is a correlation between
- 10 the reflection coefficient measured by the protein error indicator and the protein concentration and therefore, it is possible to measure the protein concentration by measuring the reflection coefficient. The correlation between the reflection coefficient (x(%)) and the protein concentration
- 15 (y(mg/dL)) can be expressed by the following Mathematical Formula 1 using the least-square method.

Mathematical Formula 1

$$y = 2 * 10^9 * x^{-4.4653}$$

20 Example 2

In the present example, a plurality of liquid samples each having a different creatinine concentration from others were used, to study how the amount of creatinine influences the actual measurement of protein concentration.

- 25 The test paper was made following the same procedure as in Example 1. The reflection coefficients were measured by colorimeter, based on a reflected light when the test paper

was irradiated with a light whose peak wavelength was 630 nm.

The protein concentrations were calculated by assigning the measured reflection coefficients to Mathematical Formula 1. On the other hand, the amounts of creatinine were measured by an enzyme method. In the enzyme method, creatinine amidohydrolase was used as the enzyme to generate creatine. Thereafter, creatine amidohydrolase, sarcosine oxidase and peroxidase were added to the creatine, then the amount of creatine was quantified conventionally, in accordance with the standard method, and creatinine concentration was determined from the amount of creatine.

The liquid samples used had the same protein concentration and different creatinine concentration from each other. Each liquid sample was made by adding an appropriate amount of creatinine to low-creatinine-concentration, healthy-human urine which had a protein concentration of 5.3 mg/dL approx., and a creatinine concentration not higher than 20 mg/dL. The amount of the liquid sample dripped to the test paper was 7 μ L.

Results of the measurements on the creatinine concentrations and protein concentrations are given in Fig. 2, where the creatinine concentration is represented by the horizontal axis, and the protein concentration is represented by the vertical axis, using the symbol (\diamond). As understood from Fig. 2, with the actual protein concentration being consistent, a greater creatinine concentration will cause Mathematical Formula 1 to give a proportionally greater protein concentration. Specifically, it is observed that the reflection coefficient which is measured as a result of

reaction between creatinine and the protein error indicator
TBPB decreases whereas the calculated value is higher than
the protein concentration. This means that once the
creatinine concentration is found, it is possible to tell how
5 much higher the calculated value is than the actual protein
concentration, i.e. it is possible to tell the creatinine
influence quantity.

Now, the relationship between the creatinine
concentration (x (mg/dL)) in Fig. 2 and the calculated protein
10 concentration (y (mg/dL)) based on Mathematical Formula 1 can
be expressed by a proportional expression as the following
Mathematical Formula 2, using the least-square method.

Mathematical Formula 2

$$y = 0.0051x + 5.3076$$

15

Further, the protein concentration (Y (mg/dL)) which is
the value after eliminating the influence caused by the amount
of creatinine can be given by the following Formula 3.

20 Mathematical Formula 3

$$Y = y - 0.0051x$$

Now, healthy urine has an average creatinine concentration
of 100 mg/dL. With this being a standard, the above
Mathematical Formula 3 can be expressed as the following
25 Mathematical Formula 4.

Mathematical Formula 4

$$Y=y-0.0051(x-100)$$

Fig. 2 also plots protein concentrations calculated by Mathematical Formula 4, using the symbol (\diamond). The protein concentrations calculated by Mathematical Formula 4 are substantially consistent regardless of the creatinine concentration, indicating that the influence from the amount of creatinine is eliminated.

10 Example 3

In the present example, a halogenated xanthene dye was carried in test paper. Liquid samples are dripped onto the test paper, and relationship between reflection coefficients and albumin concentrations measured by the immunoturbidimetric method was studied.

The test paper was made by the same way as in Example 1, differing only in that the protein measurement indicator was provided by a halogenated xanthene dye (Phloxine B, manufactured by Tokyo Chemical Industry Co., Ltd. (Japan)) represented by Chemical Formula 2. The reflection coefficients were measured by colorimeter, based on a reflected light when the test paper was irradiated with a light whose peak wavelength was 560 nm. The liquid samples were made in the same way as in Example 1.

The albumin concentration measurements using the immunoturbidimetric method were based quantification by means of optical absorbency observed when a light whose wavelength

was 340 nm was applied to a reaction liquid resulted from the reaction between the antibody, which was provided by the monoclonal antibody, and albumin.

Results of the measurements on the reflection coefficients and the protein concentrations are given in Fig. 3, where the reflection coefficient is represented by the horizontal axis and the albumin concentration is represented by the vertical axis. As understood from Fig. 3, there is a correlation between the reflection coefficient measured by using the halogenated xanthene dye and the albumin concentration. Therefore, it is possible to obtain albumin concentration by measuring the reflection coefficient. The correlation between the reflection coefficient (x(%)) and the albumin concentration (y(mg/L)) can be expressed by the following Mathematical Formula 5, using the least-square method.

Mathematical Formula 5

$$y = 8 * 10^{14} * x^{-7.2932}$$

Example 4

In the present example, a plurality of liquid samples having different creatinine concentrations were used to study influences of the amount of creatinine on the reflection coefficients (the albumin concentrations which were actually measured).

The test paper was made by the same way as in Example 3. The reflection coefficients were measured by colorimeter, based on a reflected light when the test paper was irradiated

with a light whose peak wavelength was 560 nm. The albumin concentrations were calculated by assigning the measured reflection coefficients to Mathematical Formula 5. The amounts of creatinine were measured by the enzyme method as
5 in Example 2.

The liquid samples used had the same protein concentration and different creatinine concentration from each other. Two kinds of liquid samples were made: by adding an appropriate amount of creatinine to low-creatinine-concentration,
10 healthy-human urine having a creatinine concentration not higher than 20 mg/dL (low-albumin samples); and by adding human serum albumin to the above-described healthy-human urine in addition to an appropriate amount of creatinine (high-albumin samples). The amount of the liquid sample dripped to the test
15 paper was 7 μ L.

Results of the measurements on the creatinine concentrations and reflection coefficient are given in Fig. 4. In Fig. 4, the creatinine concentration is represented by the horizontal axis and the reflection coefficient is
20 represented by the vertical axis. The measurements on the low-albumin samples are plotted with the symbol (\diamond) whereas those on the high -albumin samples are plotted with the symbol (\blacksquare). As understood from Fig. 4, with the actual albumin concentration being consistent, a greater creatinine
25 concentration will give a proportionally smaller reflection coefficient. The result means that creatinine reacts with the halogenated xanthene dye, decreasing the measured reflection coefficient while increasing the calculated value beyond the actual protein concentration. Simultaneously,

this means that once the creatinine concentration is found, it is possible to tell how much higher the calculated value is than the actual protein concentration, i.e. it is possible to tell the creatinine influence quantity.

5 Now, the relationship between the creatinine concentration (x (mg/dL)) and the reflection coefficient (y (%)) can be expressed by Mathematical Formula 6(1) for the low-albumin samples and by Mathematical Formula 6(2) for the high-albumin samples, using the least-square method.

10

Mathematical Formulas 6

$$y = -0.0188x + 89.135 \dots (1)$$

$$y = -0.0158x + 70.837 \dots (2)$$

In Mathematical Formula 6-(1) and Mathematical Formula
15 6-(2), it should be noted that a different albumin concentration will give a different gradient. Specifically, in Mathematical Formula 6-(1) and Mathematical Formula 6-(2) the gradient is the index which shows the extent of influence caused by the amount of creatinine. The different gradients
20 mean that a different albumin concentration will result in a different creatinine influence quantity. This point is also understood from the fact in Fig. 3 that the relationship between albumin concentration and reflection coefficient is not linear, and there is a lower limit in the value of reflection coefficient.
25 Fig. 5 shows results of albumin concentration calculations by Mathematical Formula 5 from actually measured reflection coefficients from the low-albumin samples and the high-albumin

samples. In Fig. 5, the results from the low-albumin samples are plotted with the symbol (\diamond) whereas those from the high-albumin samples are plotted with the symbol (\circ). As understood from Fig. 5, in both of the low-albumin samples and the high-albumin samples, a greater creatinine concentration will give a greater calculated albumin concentration. In addition, the high-albumin samples are under greater influence from creatinine than the low-albumin samples. In other words, the influence from the amount of creatinine can be eliminated by correcting the measured reflection coefficient in accordance with the albumin concentration thereby canceling the creatinine influence quantity, before calculating the albumin concentration based on Mathematical Formula 5.

Fig. 6 shows a graph, where the horizontal axis represents the reflection coefficient ($x(\%)$) when the creatinine concentration is 100 mg/dL, and the vertical axis represents the absolute value of the gradient ($y(-)$) in Mathematical Formula 6(1) and Mathematical Formula 6(2). The graph in Fig. 6 can be represented by the following Mathematical Formula 7.

Mathematical Formula 7

$$y = 0.0002x + 0.0042$$

Therefore, the correction formula for the reflection coefficient ($R'(\%)$) which takes into account the influence from the amount of creatinine in accordance with albumin

concentration can be expressed as the following Mathematical Formula 8. In Mathematical Formula 8, "R" represents the reflection coefficient (%) from actual measurements whereas "Cre" represents creatinine concentration (mg/dL).

5

Mathematical Formula 8

$$R' (\%) = R + (0.0002R + 0.0042) \times Cre$$

10 With the above, and with an average creatinine concentration of 100 mg/dL in healthy urine being a standard, Mathematical Formula 8 can be expressed as the following Mathematical Formula 9.

15 Mathematical Formula 9

$$R' (\%) = R + (0.0002R + 0.0042) \times (Cre - 100)$$

Fig. 5 also shows calculation results of the albumin concentration in which the reflection coefficient was first
20 corrected by using Mathematical Formula 9 and then the albumin concentration was calculated by using Mathematical Formula 5. In Fig. 5, the symbol (♦) represents calculation results for the low-albumin samples whereas the symbol (●) represents calculation results for the high-albumin samples. As
25 understood from Fig. 5, the albumin concentrations calculated by Mathematical Formula 5 using the reflection coefficient R' corrected by Mathematical Formula 9 are substantially

consistent regardless of the creatinine concentration in both of the low-albumin samples and the high-albumin samples, indicating that the influence from the amount of creatinine is eliminated.

- 5 It is contemplated that the advantages demonstrated in Examples 1 through 4 will also be seen as long as creatinine reacts with a protein measurement indicator, i.e. when Mathematical Formula 1 and Mathematical Formula 5 are established from other methods of protein measurement, and/or
- 10 the creatinine measurement method is provided by e.g. Jaffe method, copper chelate oxidation method, palladium complex competition method, and Benedict method.

CLAIMS

1. A method of measuring a protein based on a degree of coloring occurring when a liquid sample is mixed with a protein measurement indicator,

wherein information reflecting a concentration of creatinine in the liquid sample is obtained, and then, based on the obtained information, an influence of the creatinine on a protein concentration measurement is eliminated.

10

2. The method of measuring a protein according to claim 1, the method comprising:

a first step of obtaining a first response value which reflects a protein concentration in the liquid sample, based on coloring caused by a system containing the liquid sample and the protein measurement indicator;

a second step of obtaining a second response value which reflects a creatinine concentration in the liquid sample in a system containing the liquid sample but not containing the protein measurement indicator; and

a third step of calculating a protein concentration in the liquid sample, based on the first response value and inconsideration of the second response value.

3. The method of measuring a protein according to claim 2, wherein the second step includes calculation, based on the second response value, of an influence caused by the amount of creatinine on the first response value;

the third step including calculation of a protein

concentration as a preliminary value based on the first response value, and calculation of a final protein concentration by subtracting the influence of the amount of creatinine from the preliminary value.

5

4. The method of measuring a protein according to claim 3, wherein the calculation in the second step of the creatinine influence is based on a predetermined calibration curve;

the calibration curve being prepared by measuring, in
10 accordance with a dye binding method or a protein error method, response values with a plurality of liquid samples each having an identical protein concentration with but a different creatinine concentration, and then correlating the response values with the creatinine concentrations.

15

5. The method of measuring a protein according to claim 2, wherein in the third step, a corrected response value is obtained by correcting the first response value based on the first and the second response values, and the protein
20 concentration in the liquid sample is calculated based on the corrected response value.

25

6. The method of measuring a protein according to claim 5, wherein the corrected response value is calculated by using
an arithmetic expression derived from a plurality of sample
groups each consisting of a plurality of liquid samples having
an identical protein concentration but different creatinine
concentration, the sample groups having different protein
concentrations, respectively,

the arithmetic expression being derived from a method including: a step of measuring a response value for each of the liquid samples in each sample group; a step of obtaining a relationship between the response values from the liquid
5 samples and the creatinine concentrations in each sample group, as a plurality of relational expressions for all of the sample groups in the form of linear expression; and a step of obtaining a relationship between a gradient in each of the relational expressions and the response value from the liquid sample
10 having a specific creatinine concentration in each sample group, in the form of relational expression.

7. The method of measuring a protein according to claim 2, wherein the measurement of the first response value in the
15 first step is made in accordance with a first protein measurement procedure provided by a dye binding method or a protein error method.

8. The method of measuring a protein according to claim 2,
20 wherein the measurement of the second response value in the second step is made in accordance with an enzyme method, Jaffe method, copper chelate oxidation method, palladium complex competition method or Benedict method.

25 9. The method of measuring a protein according to claim 7, wherein the protein concentration calculation in the third step is based on a predetermined calibration curve,

the calibration curve being made by a method including:
a step of obtaining a plurality of responses for the respective


liquid samples based on the first protein measurement procedure; a step of measuring a protein concentration in the liquid samples based on a second protein measurement procedure which is less susceptible to creatinine influence than the first protein measurement procedure; and a step of relating the responses to the protein concentrations measured by the second protein measurement procedure.

10. The method of measuring a protein according to claim 9, wherein the second protein measurement procedure is provided by an immunoturbidimetric method, immunolateral agglutination method or ternary complex method.

11. The method of measuring a protein according to claim 7, wherein the protein measurement indicator is provided by a xanthene dye or a triphenylmethane dye.

12. The method of measuring a protein according to claim 11, wherein the xanthene dye is a halogenated xanthene dye which has a chemical structure expressed in the following Chemical Formula 1;

Chemical Formula 1

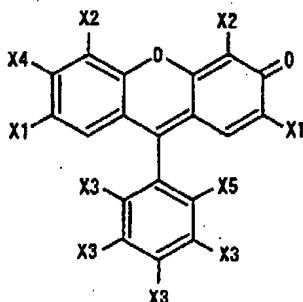


(In Chemical Formula 1, X1 represents a halogen, a nitro group or a nitroso group, X2 represents a halogen, X3 represents a halogen or hydrogen, X4 represents a hydroxyl group or its salt, and X5 represents a carboxyl group or its salt.)

5


13. The method of measuring a protein according to claim 12, wherein the halogenated xanthene dye has a chemical structure represented by a selected one of the following Chemical formulas 2 through 6:

10

Chemical Formula 2

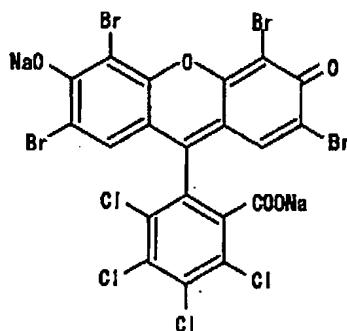


Chemical Formula 3

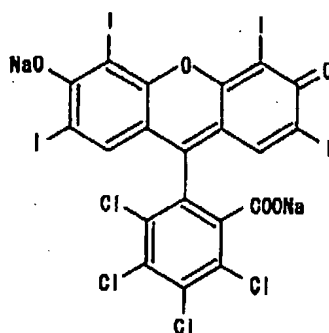


15

Chemical Formula 4

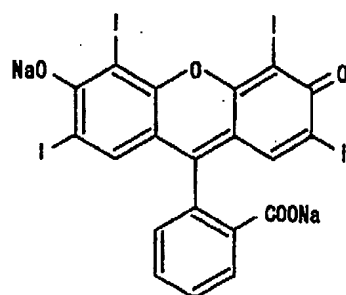


Chemical Formula 5

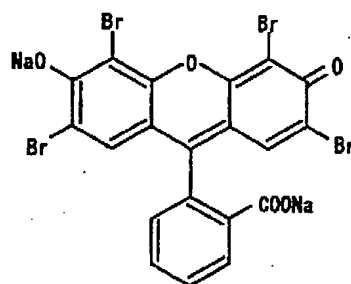

5

Chemical Formula 6

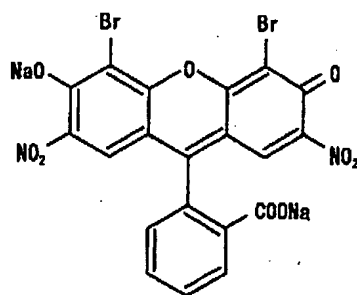

14. The method of measuring a protein according to claim 11, wherein the triphenylmethane dye is provided by Tetrabromophenol Blue (TBPB), Bromochlorophenol Blue (BCPB) or Bromophenol Blue (BPB).

5

15. The method of measuring a protein according to claim 1, wherein the protein measurement indicator is carried by a carrier in a dried form before being exposed to the liquid sample.

10

16. The method of measuring a protein according to claim 1, wherein the protein is provided by albumin.

17. The method of measuring a protein according to claim 1,
15 wherein the liquid sample is provided by urine, blood, or cerebrospinal fluid.

ABSTRACT

The present invention relates to a technique of measuring a protein based on a degree of coloring in a liquid sample mixed with a protein measurement indicator. In the present invention, information reflecting creatinine concentration in the liquid sample is obtained, and then an influence quantity caused by creatinine to the protein concentration measurement is eliminated based on the information.

FIG. 1

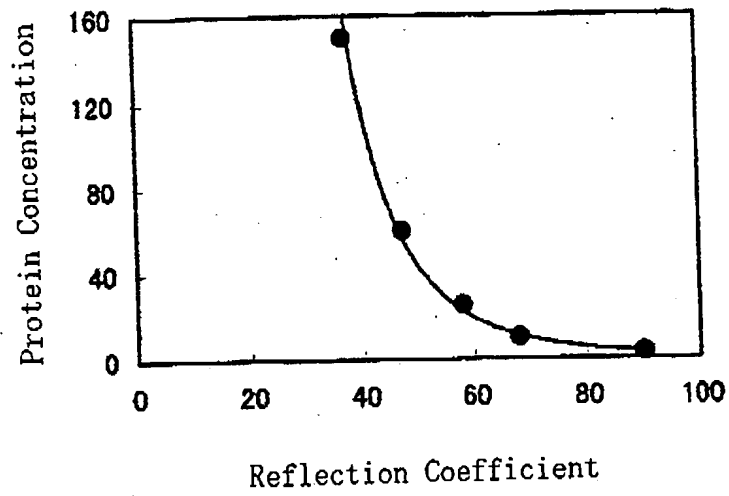


FIG. 2

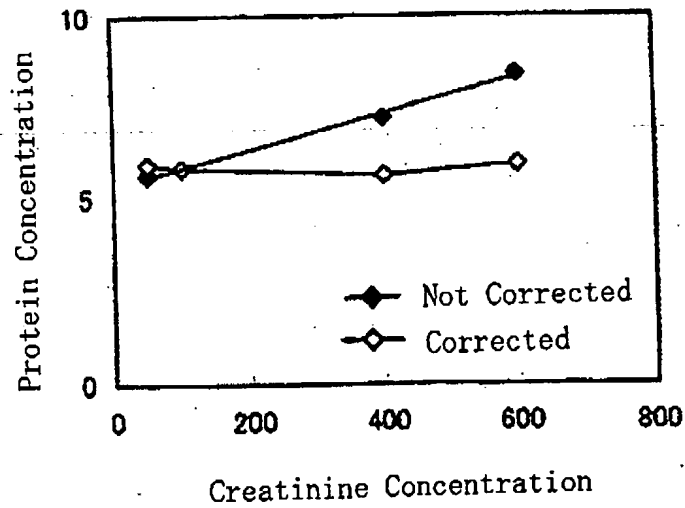


FIG. 3

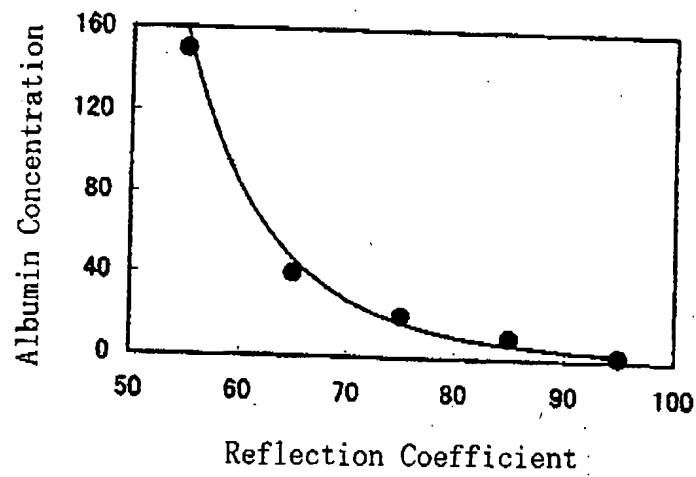


FIG. 4

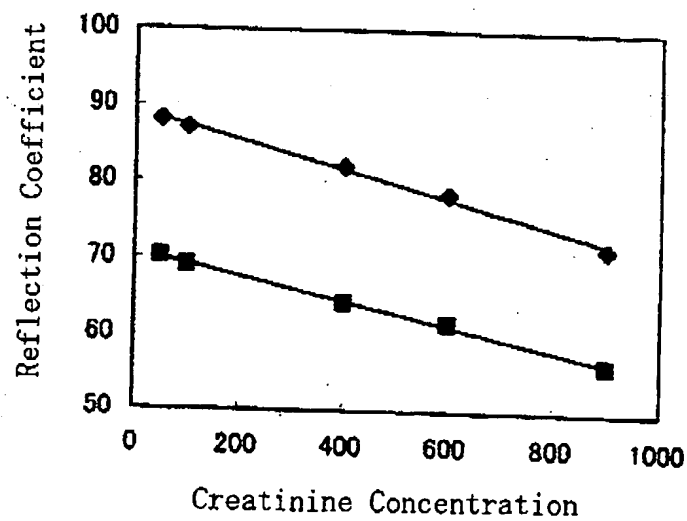


FIG. 5


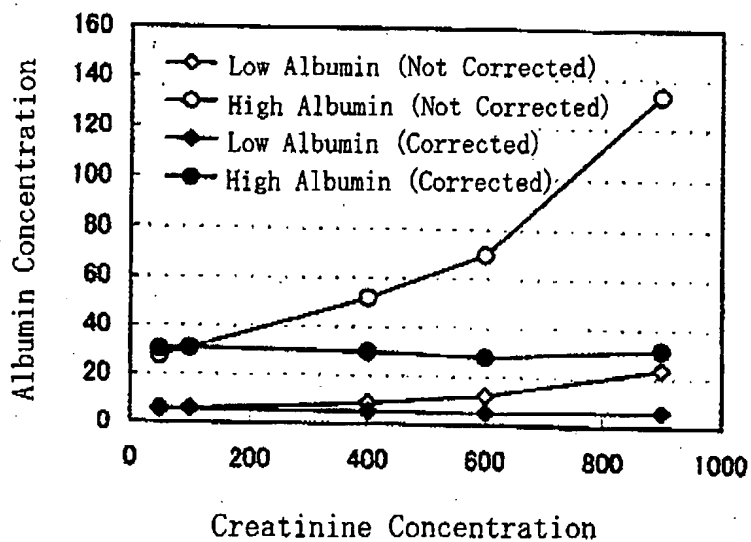


FIG. 6

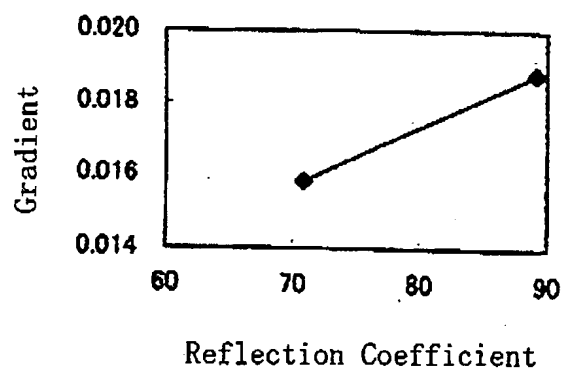

CLAIMS

1. A method of measuring a protein based on a degree of coloring occurring when a liquid sample is mixed with a protein measurement indicator,

wherein information reflecting a concentration of creatinine in the liquid sample is obtained, and then, based on the obtained information, an influence of the creatinine on a protein concentration measurement is eliminated.

10

2. The method of measuring a protein according to claim 1, the method comprising:

a first step of obtaining a first response value which reflects a protein concentration in the liquid sample, based on coloring caused by a system containing the liquid sample and the protein measurement indicator;

a second step of obtaining a second response value which reflects a creatinine concentration in the liquid sample in a system containing the liquid sample but not containing the protein measurement indicator; and

a third step of calculating a protein concentration in the liquid sample, based on the first response value and inconsideration of the second response value.

3. The method of measuring a protein according to claim 2, wherein the second step includes calculation, based on the second response value, of an influence caused by the amount of creatinine on the first response value;

the third step including calculation of a protein

concentration as a preliminary value based on the first response value, and calculation of a final protein concentration by subtracting the influence of the amount of creatinine from the preliminary value.

5

4. The method of measuring a protein according to claim 3, wherein the calculation in the second step of the creatinine influence is based on a predetermined calibration curve;

the calibration curve being prepared by measuring, in
10 accordance with a dye binding method or a protein error method, response values with a plurality of liquid samples each having an identical protein concentration with but a different creatinine concentration, and then correlating the response values with the creatinine concentrations.

15

5. The method of measuring a protein according to claim 2, wherein in the third step, a corrected response value is obtained by correcting the first response value based on the first and the second response values, and the protein
20 concentration in the liquid sample is calculated based on the corrected response value.

6. The method of measuring a protein according to claim 5, wherein the corrected response value is calculated by using
25 an arithmetic expression derived from a plurality of sample groups each consisting of a plurality of liquid samples having an identical protein concentration but different creatinine concentration, the sample groups having different protein concentrations, respectively,

the arithmetic expression being derived from a method including: a step of measuring a response value for each of the liquid samples in each sample group; a step of obtaining a relationship between the response values from the liquid
5 samples and the creatinine concentrations in each sample group, as a plurality of relational expressions for all of the sample groups in the form of linear expression; and a step of obtaining a relationship between a gradient in each of the relational expressions and the response value from the liquid sample
10 having a specific creatinine concentration in each sample group, in the form of relational expression.

7. The method of measuring a protein according to claim 2, wherein the measurement of the first response value in the
15 first step is made in accordance with a first protein measurement procedure provided by a dye binding method or a protein error method.

8. The method of measuring a protein according to claim 2,
20 wherein the measurement of the second response value in the second step is made in accordance with an enzyme method, Jaffe method, copper chelate oxidation method, palladium complex competition method or Benedict method.

25 9. The method of measuring a protein according to claim 7, wherein the protein concentration calculation in the third step is based on a predetermined calibration curve,

the calibration curve being made by a method including:
a step of obtaining a plurality of responses for the respective


liquid samples based on the first protein measurement procedure; a step of measuring a protein concentration in the liquid samples based on a second protein measurement procedure which is less susceptible to creatinine influence than the first protein measurement procedure; and a step of relating the responses to the protein concentrations measured by the second protein measurement procedure.

10. The method of measuring a protein according to claim 9, wherein the second protein measurement procedure is provided by an immunoturbidimetric method, immunol latex agglutination method or ternary complex method.

11. The method of measuring a protein according to claim 7, wherein the protein measurement indicator is provided by a xanthene dye or a triphenylmethane dye.

12. The method of measuring a protein according to claim 11, wherein the xanthene dye is a halogenated xanthene dye which has a chemical structure expressed in the following Chemical Formula 1;

Chemical Formula 1

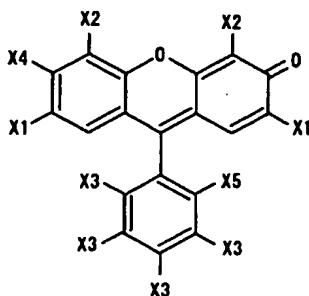


(In Chemical Formula 1, X1 represents a halogen, a nitro group or a nitroso group, X2 represents a halogen, X3 represents a halogen or hydrogen, X4 represents a hydroxyl group or its salt, and X5 represents a carboxyl group or its salt.)

5


13. The method of measuring a protein according to claim 12, wherein the halogenated xanthene dye has a chemical structure represented by a selected one of the following Chemical formulas 2 through 6:

10

Chemical Formula 2

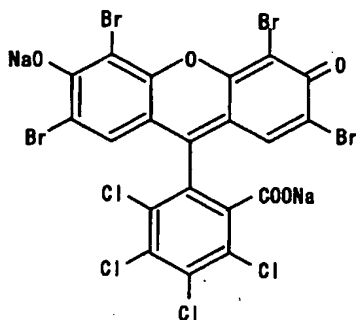


Chemical Formula 3

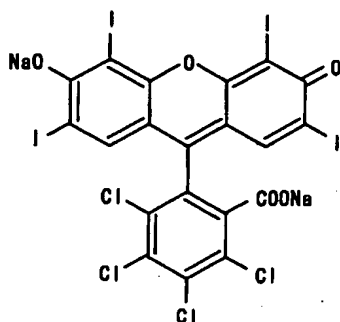


15

Chemical Formula 4

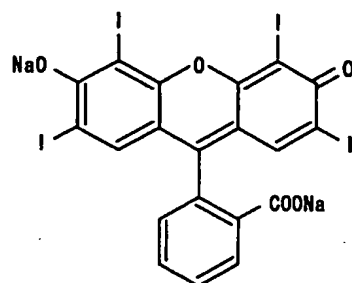


Chemical Formula 5

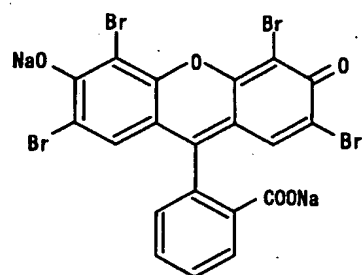

5

Chemical Formula 6

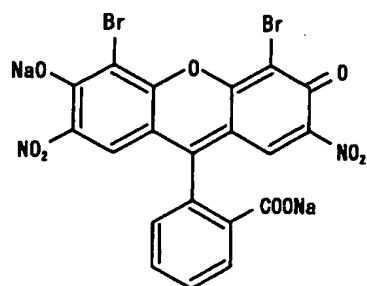

14. The method of measuring a protein according to claim 11, wherein the triphenylmethane dye is provided by Tetrabromophenol Blue (TBPB), Bromochlorophenol Blue (BCPB) or Bromophenol Blue (BPB).

5

15. The method of measuring a protein according to claim 1, wherein the protein measurement indicator is carried by a carrier in a dried form before being exposed to the liquid sample.

10

16. The method of measuring a protein according to claim 1, wherein the protein is provided by albumin.

17. The method of measuring a protein according to claim 1,
15 wherein the liquid sample is provided by urine, blood, or cerebrospinal fluid.